

(12)

(21) 2 422 950

(51) Int. Cl. ⁷: **G06K 9/00**

(22) 25.09.2001

(85) 25.03.2003

(86) PCT/US01/30038

(87) WO02/035454

(30) 60/234,376 US 25.09.2000

(71) Z-KAT, INC.,
2903 Simms Street, HOLLYWOOD, XX (US).


(72) SANTOS-MUNNE, JULIO J. (US).
ABOVITZ, RONY A. (US).
LAROCQUE, BRANDON D. (US).

(74) KIRBY EADES GALE BAKER

(54) ARTEFACT DE CALAGE D'IMAGES PAR FLUORESCENCE A MARQUEURS OPTIQUES ET/OU MAGNETIQUES
(54) FLUOROSCOPIC REGISTRATION ARTIFACT WITH OPTICAL AND/OR MAGNETIC MARKERS

(57)

A registration artifact (10) for use in registering two or more fluoroscopic images includes a plurality of radio opaque spheres (12, 14, 16) and a plurality of trackable markers, such as optical reflectors (20, 22, 24, and 26), mounted to a radio transparent body (11). A tracking system locates the position of registrable artifact using the trackable markers for registering the fluoroscopic images with respect to a known frame of reference.

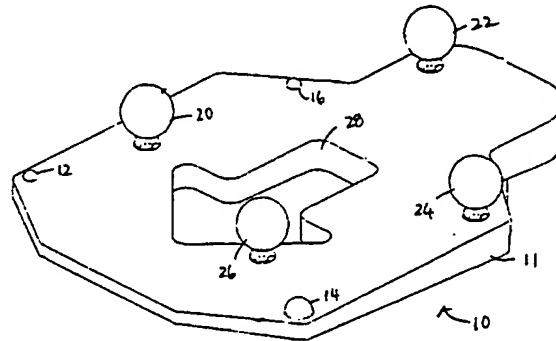



Office de la Propriété
Intellectuelle
du Canada

Un organisme
d'Industrie Canada

Canadian
Intellectual Property
Office

An agency of
Industry Canada

CA 2422950 A1 2002/05/02

(21) 2 422 950

(12) DEMANDE DE BREVET CANADIEN
CANADIAN PATENT APPLICATION

(13) A1

(86) Date de dépôt PCT/PCT Filing Date: 2001/09/25

(87) Date publication PCT/PCT Publication Date: 2002/05/02

(85) Entrée phase nationale/National Entry: 2003/03/25

(86) N° demande PCT/PCT Application No.: US 2001/030038

(87) N° publication PCT/PCT Publication No.: 2002/035454

(30) Priorité/Priority: 2000/09/25 (60/234,376) US

(51) Cl.Int.⁷/Int.Cl.⁷ G06K 9/00


(71) Demandeur/Applicant:
Z-KAT, INC., US

(72) Inventeurs/Inventors:
ABOVITZ, RONY A., US;
LAROCQUE, BRANDON D., US;
SANTOS-MUNNE, JULIO J., US

(74) Agent: KIRBY EADES GALE BAKER

(54) Titre : ARTEFACT DE CALAGE D'IMAGES PAR FLUORESCENCE A MARQUEURS OPTIQUES ET/OU
MAGNETIQUES

(54) Title: FLUOROSCOPIC REGISTRATION ARTIFACT WITH OPTICAL AND/OR MAGNETIC MARKERS

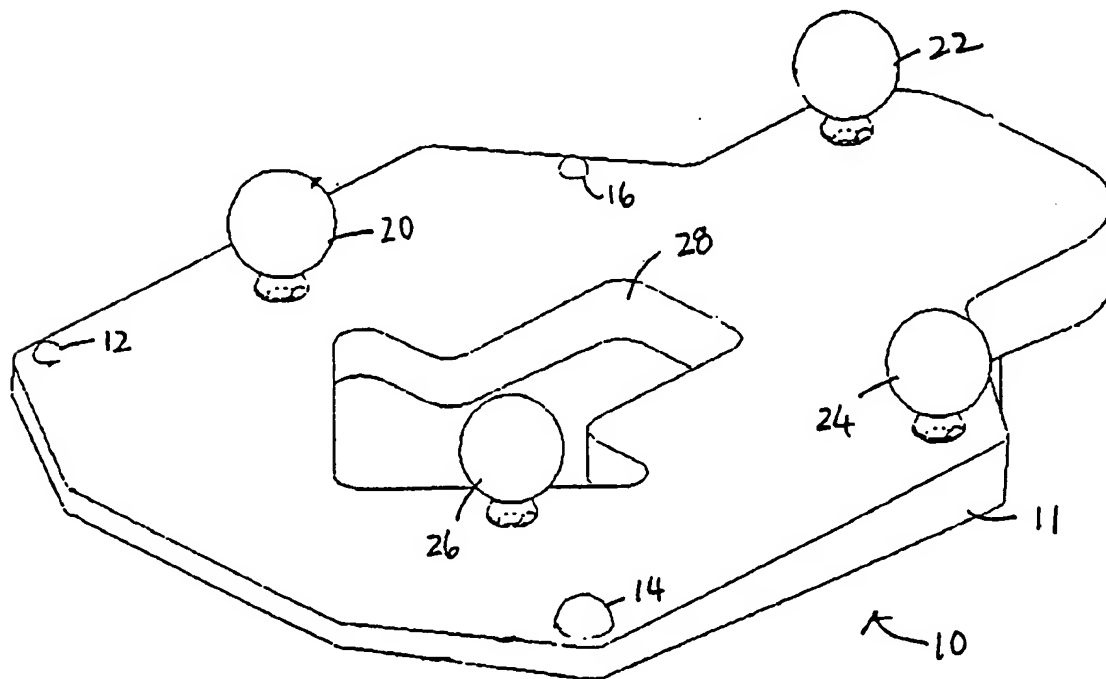

(57) Abrégé/Abstract:

A registration artifact (10) for use in registering two or more fluoroscopic images includes a plurality of radio opaque spheres (12, 14, 16) and a plurality of trackable markers, such as optical reflectors (20, 22, 24, and 26), mounted to a radio transparent body (11). A tracking system locates the position of registrable artifact using the trackable markers for registering the fluoroscopic images with respect to a known frame of reference.

Canada

<http://opic.gc.ca> • Ottawa-Hull K1A 0C9 • <http://cipo.gc.ca>

OPIC • CIPQ 191

OPIC



CIPO

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

CORRECTED VERSION

(19) World Intellectual Property Organization
International Bureau(43) International Publication Date
2 May 2002 (02.05.2002)


PCT

(10) International Publication Number
WO 02/035454 A1

- (51) International Patent Classification⁷: **G06K 9/00**
- (21) International Application Number: **PCT/US01/30038**
- (22) International Filing Date:
25 September 2001 (25.09.2001)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
60/234,376 25 September 2000 (25.09.2000) US
- (71) Applicant: **Z-KAT, INC.** [US/US]; 2903 Simms Street, Hollywood, FL 33020 (US).
- (72) Inventors: **ABOVITZ, Rony, A.**; 3825 Taft Street, Hollywood, FL 33021 (US). **LAROCQUE, Brandon, D.**; 761 SW 148th Avenue #912, Sunrise, FL 33325 (US). **SANTOS-MUNNE, Julio, J.**; 1750 Henley Road, Unit 23, Glenview, IL 60025 (US).
- (74) Agents: **HUBBARD, Marc, A. et al.**; Munsch Hardt Kopf & Harr, P.C., 1445 Ross Avenue, Suite 4000, Dallas, TX 75202-2790 (US).
- (81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PH, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.
- (84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:
— with international search report

[Continued on next page]

(54) Title: FLUOROSCOPIC REGISTRATION ARTIFACT WITH OPTICAL AND/OR MAGNETIC MARKERS

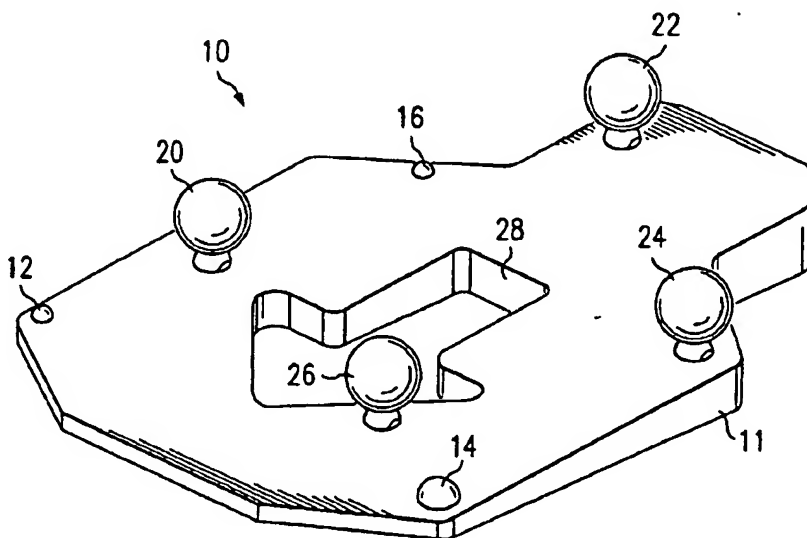

(57) Abstract: A registration artifact (10) for use in registering two or more fluoroscopic images includes a plurality of radio opaque spheres (12, 14, 16) and a plurality of trackable markers, such as optical reflectors (20, 22, 24, and 26), mounted to a radio transparent body (11). A tracking system locates the position of registrable artifact using the trackable markers for registering the fluoroscopic images with respect to a known frame of reference.

WO 02/035454 A1

WO 02/035454 A1



(48) Date of publication of this corrected version:

20 March 2003

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(15) Information about Correction:

see PCT Gazette No. 12/2003 of 20 March 2003, Section II

FLUOROSCOPIC REGISTRATION ARTIFACT WITH OPTICAL AND/OR MAGNETIC MARKERS

TECHNICAL FIELD OF THE INVENTION

The invention relates to image guided surgical and interventional systems.

BACKGROUND OF THE INVENTION

5 Conventional fluoroscopic registration artifacts have X-ray transparent bodies holding radio-opaque fiducials in predetermined and fixed positions on the registration artifact. The fiducials show up as distinct dots on an X-ray and used to coordinate and register to a common coordinate system multiple X-ray images of a patient taken from different perspectives. The registration artifact remains fixed in position from one image to the next in order to register the
10 images, as an assumption is made that the fiducials in the respective images are in the same positions.

 In certain situations, it is advantageous or necessary to relocate the registration artifact. For example, in some instances it is difficult to fit the registration artifact and the relevant anatomy within the fluoroscopic field in the fluoroscopic images due to the particular anatomy or
15 physical configuration of the patient. An obese patient may present such challenges, for example.

 One solution has been to track the position of fluoroscope in an operating room rather than use a registration artifact. However, tracking the fluoroscope requires expensive modifications to the fluoroscope.

20 SUMMARY OF THE INVENTION

 According to the invention, fluoroscopic images are registered using a registration artifact that may be relocated. The registration artifact, in which a plurality of radio-opaque fiducials are mounted in a known geometric relationship, includes a plurality of markers having a known relationship to the artifact. The positions of the markers, and thus the position of the
25 registration artifact, are tracked by a tracking system. Examples of such tracking systems include passive and active optical, magnetic and acoustic systems. The position of the registration artifact with respect to a known coordinate frame is determined by the tracking system. Therefore, the registration artifact need not be kept in a fixed location in order to register the images. Rather, the registration artifact may be moved as necessary to fit the registration artifact
30 into an image, and no modification of the fluoroscope is necessary.

BRIEF DESCRIPTION OF THE DRAWINGS

For a more complete understanding of the present invention, the objects and advantages thereof, reference is now made to the following descriptions taken in connection with the accompanying drawings in which:

- 5 FIGURE 1 is a perspective view of an embodiment of a registration artifact;
FIGURE 2 is a perspective view of a second embodiment of a registration artifact;
FIGURE 3 is a diagram showing the registration artifact being located over a relevant anatomy of a patient with a drill guide according to the teachings of the present invention;
FIGURE 4 is a diagram showing some of the tools that may be used in conjunction with
10 the registration artifact according to the teachings of the present invention; and
FIGURE 5 is a diagram showing an operating room set up according to the teachings of the present invention.

DETAILED DESCRIPTION OF THE DRAWINGS

- 15 The preferred embodiment of the present invention and its advantages are best understood by referring to FIGURES 1 through 5 of the drawings, like numerals being used for like and corresponding parts of the various drawings in a known geometric relationship.

Referring to FIG. 1, registration artifact 10 includes a radio-transparent body 11 upon which radio-opaque fiducials 12-16 are mounted. Also mounted to the registration artifact 10 are
20 a plurality of markers 20-26 that may be located and tracked using a tracking system. For example, trackable markers 20-26 may be active infrared emitting diodes (IREDs), reflective spheres, magnetically trackable objects, or other spacially trackable objects. Registration artifact 10 may also include a direction indicator 28 to aid in the positioning of the artifact for a procedure. In the embodiment shown, direction indicator 28 is an opening in the shape of an
25 arrow formed in the body 11 of registration artifact 10.

Optically trackable markers may be imaged and tracked in the infrared spectrum or visible spectrum by cameras. The location of magnetically trackable markers are detected by measuring the disturbance of the magnetic field. The cameras and detectors have a much wider field of "view" than the typical fluoroscopy images. An advantage of using magnetic markers is
30 that a line-of-sight between the camera/detector and each of the markers is not required. This may provide more flexibility in how the surgical instruments, robotic arms that assist with surgery, the patient, and a surgical team are positioned.

Referring to FIG. 2, a second embodiment of a registration artifact 30, like the registration artifact of FIG. 1, includes a plurality of radio-opaque fiducials 32 arranged in a predetermined geometric relationship and a plurality trackable markers 34 arranged in a known geometric relationship.

5 Referring to FIGS. 3-5, registration artifact 30 is mounted on a bracket 36 that clamps to a table 38 on which torso 40 of a patient rests. The bracket allows the artifact to be positioned in the field of view of C-arm fluoroscope 66. The registration artifact may be placed in any other suitable structure. As an example only, drill guide 42 is placed adjacent an entry opening in the patient's torso with a drill 43 being inserted. The drill guide includes a frame on which a
10 plurality of trackable markers, in the form of infrared reflective spheres 44, are attached in a known geometric relationship to the axis and end point of the drill guide. The position of the axis and end point of the drill guide are registered to fluoroscopic images taken with registration artifact 30 in the field of view.

Referring only to FIG. 4, elements of an image guide surgical system include an optical
15 tracking system and related surgical instruments. Optical tracking systems are well known. Other types of tracking systems include magnetic, fiber-optic and acoustic tracking systems. Optical tracking systems typically include a camera system 46 that senses the positions of trackable markers within its field of view that transmit or reflect infrared or other electro-magnetic radiation that is not harmful to persons. The signals from optical camera system are processed
20 using a program running on computer 48. The programs locate the positions of trackable markers and determine the position of an object to which the markers are attached with respect to a known coordinate system or reference frame. This position can be used by the computer to generate, for example, a representation of the object that is displayed on a fluoroscopic image of the patient in an accurate spatial relationship with the patient's anatomy for guiding the
25 positioning of the object. The computer includes a keyboard 50 and trackball 52, both of which function as input devices, a monitor 54 for display images and a backup power supply. Surgical instruments include in addition to drill guide 42, probes 58 and 60. These instruments are mounted with trackable markers. Tracker 62 also includes a plurality of trackable markers mounted in a known relationship. It may be clamped to other objects that do not have integrally
30 mounted trackable markers.

Referring back to FIGS. 3-5, fluoroscopic images of the patient's anatomy are captured from at least two different angles using C-arm fluoroscope with a registration artifact in the field

of view. As explained in U.S. Patent No. 5,799,055, entitled *Apparatus and Method for Planning a Stereotactic Surgical Procedure Using Coordinated Fluoroscopy*, issued on Aug. 25, 1998 to Peshkin et al., which is incorporated herein by reference, the fluoroscopic images are registered by locating the positions of the fiducials in the images. However, using this method requires the
5 fiducials to remain in the same position.

When registration artifact 10 is used, the registration artifact no longer needs to remain in a same position in multiple fluoroscopic images. The position of markers on the registration artifact is tracked between images using a tracking system, such as the optical tracking system shown in the figures or other type of tracking system, depending on the type of trackable markers
10 used. This information is used to adjust or compensate for the movement of the registration artifact between the images when registering multiple fluoroscopic images. Therefore, the position of the registration artifact in each image is known. The registration artifact can even be moved to another object, such as a surgical tool on the end of a robotic arm, and its new location tracked and calculated relative to the relevant anatomy of the patient.



15 While the invention has been particularly shown and described by the foregoing detailed description, it will be understood by those skilled in the art that various changes, alterations, modifications, mutations and derivations in form and detail may be made without departing from the spirit and scope of the invention.

What is claimed is:

Claims:

1. Registration artifact for use in registering fluoroscopic images comprising:
a plurality of radio-opaque fiducials arranged in a known geometric relationship; and
a plurality of trackable markers disposed on the artifact in a known geometric
5 relationship to fiducials.
2. A method for registering fluoroscopic images comprising:
capturing a first fluoroscopic image of a patient and a registration artifact from a first
perspective, the registration artifact including, a plurality of radio-opaque fiducials arranged in a
10 known geometric relationship and a plurality of trackable markers disposed in a known
geometric relationship to fiducials;
determining the position of the registration artifact in the first fluoroscopic image with
respect to a known coordinate frame by determining the position of the markers using the
tracking system; and
15 capturing a second fluoroscopic image of the patient and the registration artifact frame
second perspective;
determining the position of the registration artifact in the second fluoroscopic image with
respect to the known coordinate frame by determining the position of the markers using the
tracking system;
20 registering the first and second fluoroscopic images using the positions of the fiducials in
each fluoroscopic image and the determined positions of the registration artifact.
registering the fluoroscopic images.

1/3

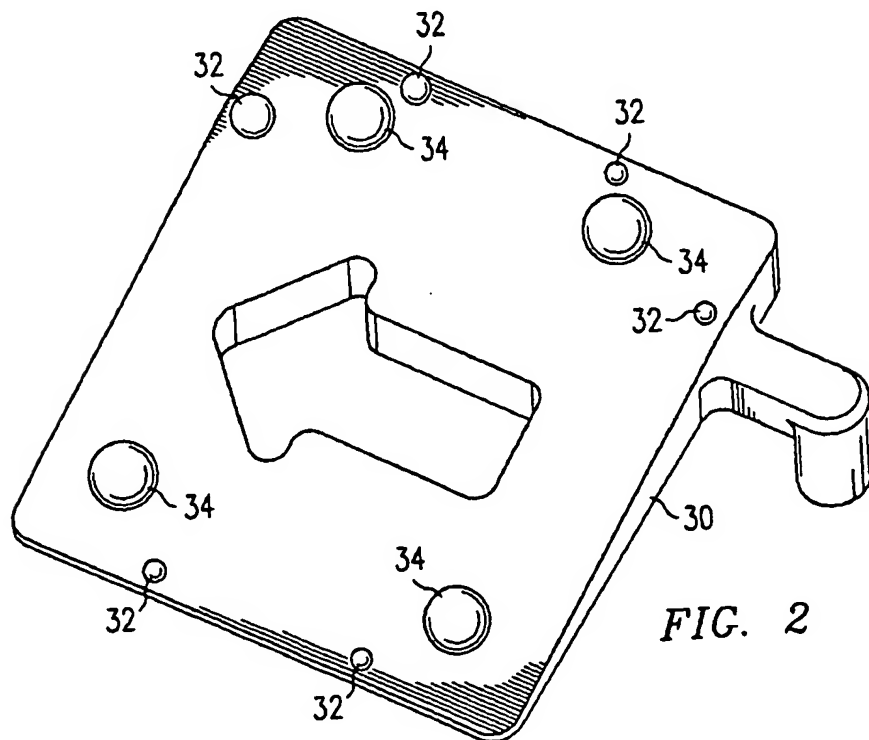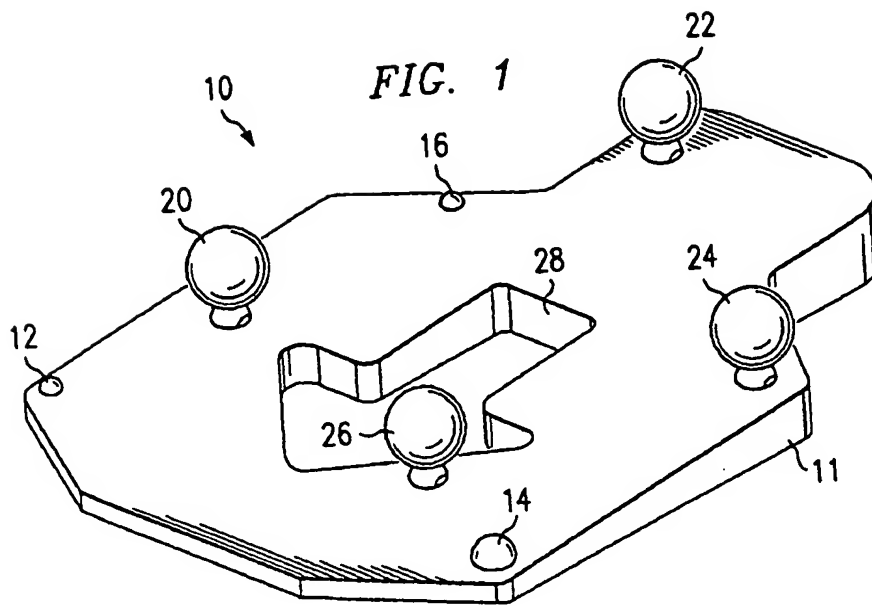

2/3

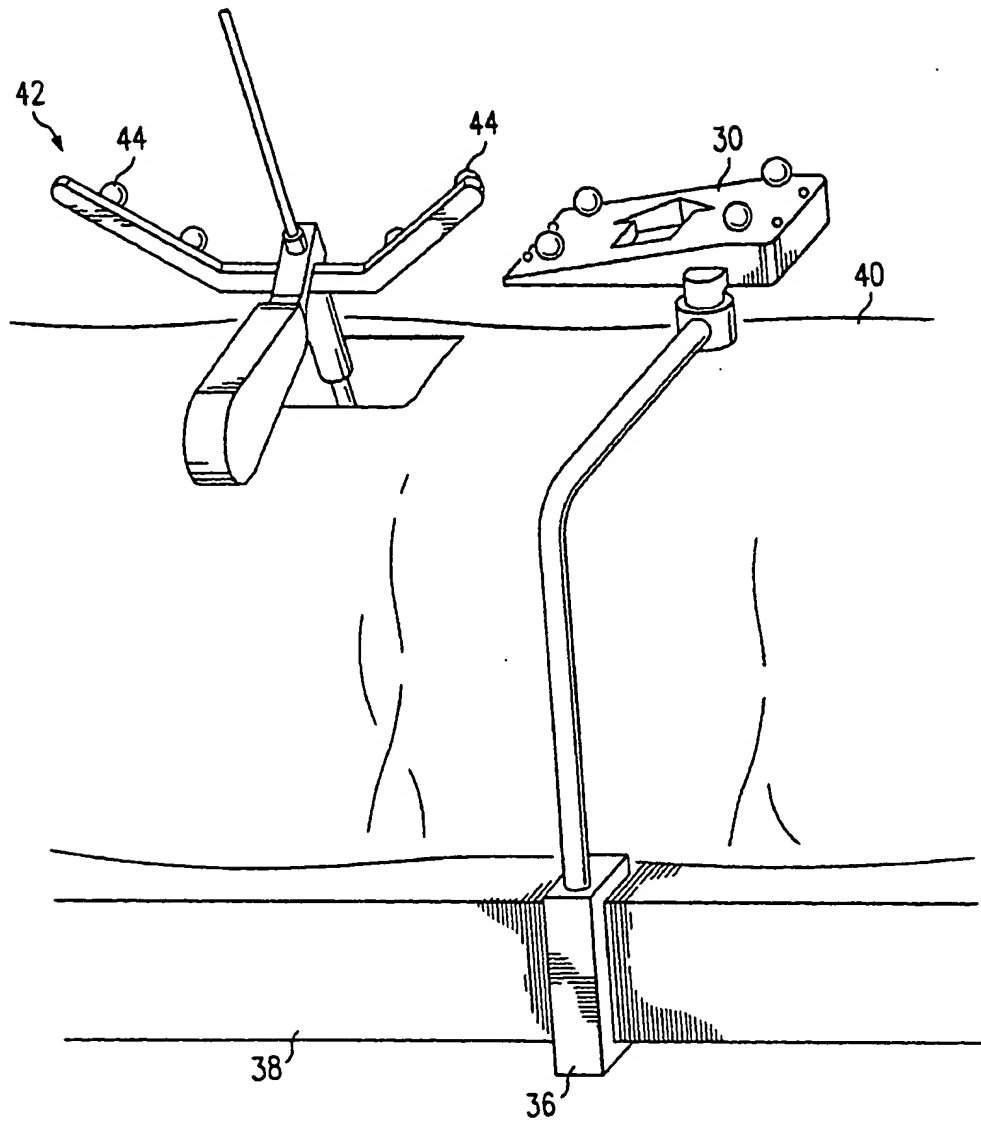


FIG. 3

3/3

